




iHealth[®] Edge

Get motivated. Get moving. Get tracking

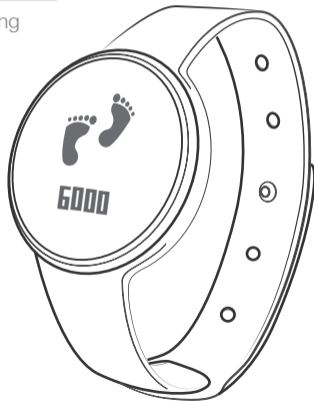

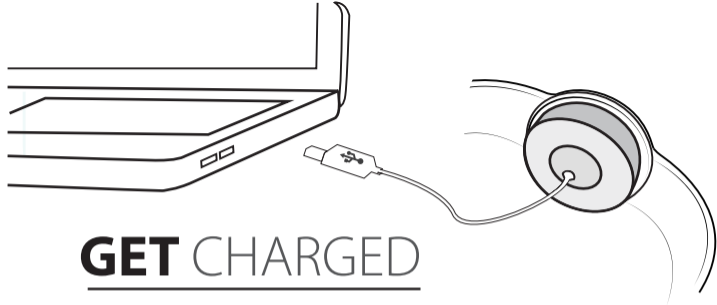


GET CHARGED

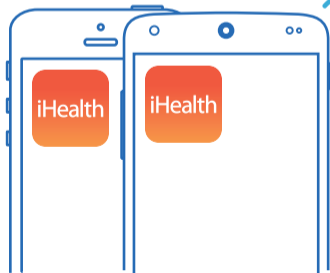

Is your mobile device compatible?
Visit www.ihealthlabs.com to check!

GET THE APP

1 Turn Bluetooth on




2 Open app




GET CONNECTED


3 Select Activity in menu


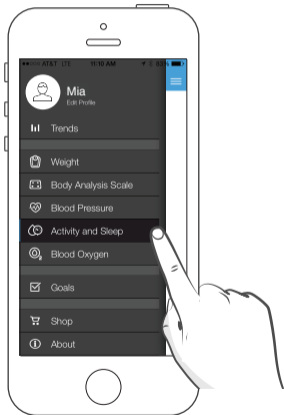


4 Click on "+" button

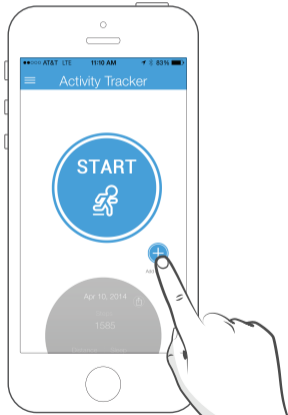


5 Select Edge

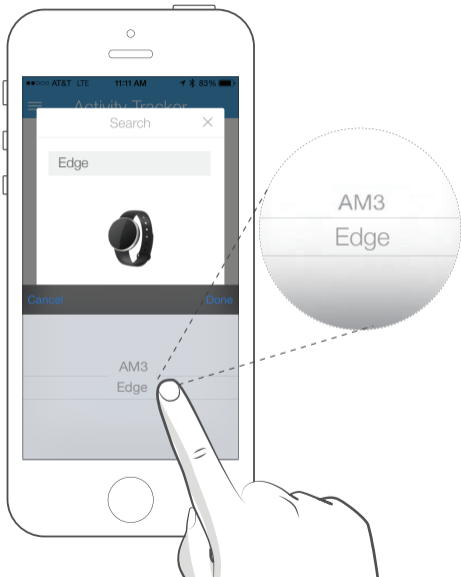

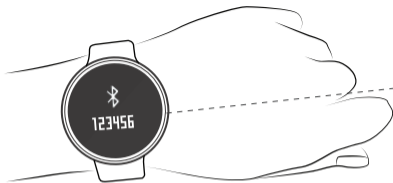


6 Enter the last 2 of 6 digits shown on tracker

If you don't see the 6 digits, turn off bluetooth and turn on again or double click the Home button (iOS) or go to the app menu (Android) and swipe over the app to fully close it. Repeat the steps from step 2.

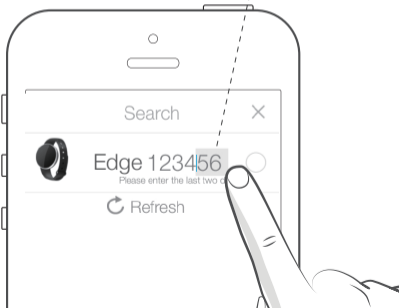


7

Pairing Successful

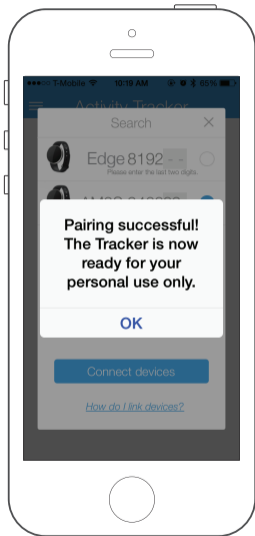

DISPLAYS

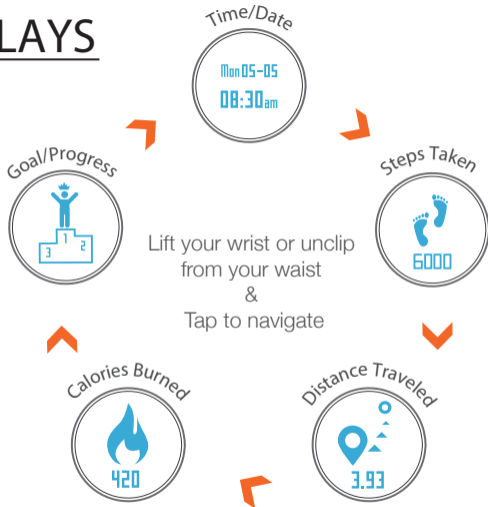

MODE



Automatically track your sleep and workout quality.

PERSONALIZE



In a different mood? Change the character on the tracker in the App settings.

IMPORTANT INFORMATION REQUIRED BY THE FCC

This device complies with part 15 of the FCC Rules. Its operation is subject to the following two conditions:

- (1) This device may not cause harmful interference, and
- (2) this device must accept any interference received, including interference that may cause undesired operation.

Changes or modifications not expressly approved by iHealth Lab Inc could void the user's authority to operate the equipment.

Note: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

This device complies with Industry Canada licence-exempt RSS standard(s). Operation is subject to the following two conditions:

- (1) this device may not cause interference, and
- (2) this device must accept any interference, including interference that may cause undesired operation of the device.



CAUTION

RISK OF EXPLOSION IF BATTERY IS REPLACED BY AN INCORRECT TYPE,
DISPOSE OF USED BATTERIES ACCORDING
TO THE INSTRUCTIONS

Hereby, [iHealth Lab Inc.], declares that this [AM3S EDGE] is in compliance with the essential requirements and other relevant provisions of Directive 1999/5/EC. Directive 1999/5/EC declaration of conformity and all iHealth certification and regulatory documents can be downloaded on the following link : <https://www.ihealthlabs.eu/support/certifications>

Contact and customer service :

Manufactured for iHealth Lab Inc.
iHealth Lab Inc.
719N. Shoreline Blvd., Mountain View, CA 94043, USA
Tel:+1-855-816-7705 www.ihealthlabs.com



Manufactured for iHealth Lab Europe.
3 rue Tronchet, 75008, Paris, France
www.ihealthlabs.eu

Manufactured by iHealth Lab Inc..
No. 3 Jinping Street, YaAn Road, Nankai District, Tianjin 300190, China.

Please visit www.ihealthlabs.com
for more information

iHealth[®] Edge