


## Instructions for Use




**1** Clean test site with isopropyl alcohol and air dry. Remove protective cap from safety lancet.

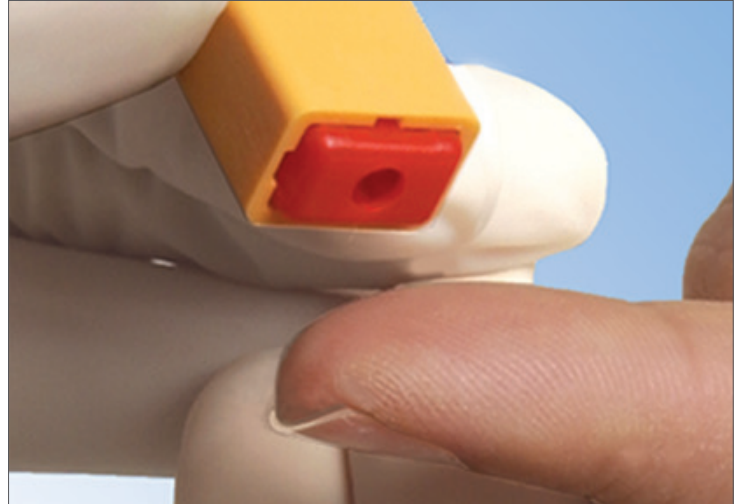

**2** Place red end of safety lancet on the test site.



**3** Push the safety lancet down against test site to activate lancet mechanism.

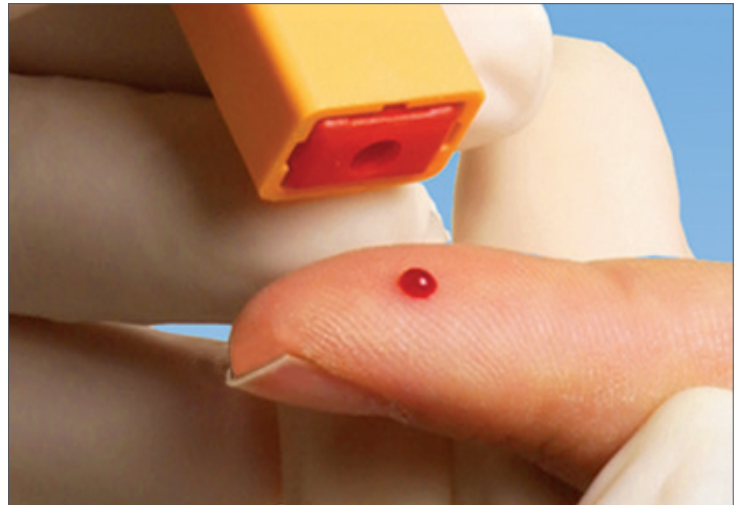

**4** Once used, simply discard lancet into a sharps container.

Single-use only. Reuse may result in patient cross-contamination.

[medipurpose.com/surgilance/ifu/](https://www.medipurpose.com/surgilance/ifu/)