

ASTA DI SOLLEVAMENTO PER DEGENTI - TUBO TONDO LIFT POLE - ROUND TUBING POTEAU DE LEVAGE - TUBE ROND SOPORTE DE ELEVACIÓN - TUBO REDONDO PENDURAL - TUBAGEM REDONDA BETTGALGEN - RUNDSTANGEN TIJĂ TELESCOPICĂ - ȚEAVĂ ROTUNDĂ LYFTPOL - RUNDRÖRSSTRUKTUR WYSIĘGNIK - Z OKRĄGŁYMI RURKAMI ANAPTHPAS EAΞHS - ΣΩΛΗΝΑΣ ΚΥΚΛΙΚΗΣ ΔΙΑΤΟΜΗΣ

È necessario segnalare qualsiasi incidente grave verificatosi in relazione al dispositivo medico da noi fornito al fabbricante e all'autorità competente dello Stato membro in cui si ha sede.

All serious accidents concerning the medical device supplied by us must be reported to the manufacturer and competent authority of the member state where your registered office is located.

Il est nécessaire de signaler tout accident grave survenu et lié au dispositif médical que nous avons livré au fabricant et à l'autorité compétente de l'état membre où on a le siège social.

Es necesario informar al fabricante y a la autoridad competente del Estado miembro en el que se encuentra la sede sobre cualquier incidente grave que haya ocurrido en relación con el producto sanitario que le hemos suministrado.

É necessário notificar ao fabricante e às autoridades competentes do Estado-membro onde ele está sediado qualquer acidente grave verificado em relação ao dispositivo médico fornecido por nós.

Jeder schwere Unfall im Zusammenhang mit dem von uns gelieferten medizinischen Gerät muss unbedingt dem Hersteller und der zuständigen Behörde des Mitgliedsstaats, in dem das Gerät verwendet wird, gemeldet werden.

Orice accident grav produs, privitor la dispozitivul medical fabricat de firma noastră, trebuie semnalat producătorului și autorității competente în statul membru pe teritoriul căruia își are sediul utilizatorul.

Det är nödvändigt att meddela tillverkaren och de behöriga myndigheterna i den berörda medlemsstaten, om alla allvarliga olyckor som inträffat i samband med den medicintekniska utrustning som levererats av oss.

Należy poinformować producenta i kompetentne władze danego Kraju członkowskiego o każdym poważnym wypadku związanym z wyrobem medycznym naszej produkcji.

Σε περίπτωση που διαπιστώσετε οποιοδήποτε σοβαρό περιστατικό σε σχέση με την ιατρική συσκευή που σας παρέχουμε θα πρέπει να το αναφέρετε στον κατασκευαστή και στην αρμόδια αρχή του κράτους μέλους στο οποίο βρίσκεστε.

REF LW10207 (GIMA 27664)



Mingguang Longway Technology Co., Ltd. No. 59 Lingji Rd., Industrial Park, Mingguang, Anhui, China Made in China



Lotus NL B.V. Koningin Julianaplein 10, 1 e Verd, 2595AA, The Hague, Netherlands

Gima S.p.A. Via Marconi, 1 - 20060 Gessate (MI) Italy gima@gimaitaly.com - export@gimaitaly.com www.gimaitaly.com







Weight Capacity: 75kgs

INTENDED USE:

Longway Medical Accessories are Medical Devices intended to compensate for a disability or inability of the bedridden user. Support device with ground base, adaptable to any bed. Structure in tubular steel painted that can be positioned according to the patient's needs and triangle with strap to adjust its height.

CAUTION (!):

• In case of damage or malfunction of your product DOT NOT use the product and please contact the authorized and trained representative.

• Do not use the product for a purpose not indicated in this manual

 LONGWAY Medical declines all responsibilities for any consequences resulting from an incorrect use of this product and from unauthorized alteration to the frame of the product.

• LONGWAY Medical reserves the right to change the information contained in this document without previous notice

• There is a ± 3%. Deviation for the Dimensions of the Products.

GENERAL SAFETY WARNINGS:

- If you don't read this user manual, it is preferable not to use this product or another available part. If you don't understand the usage or the precautions, please contact with the dealer or the proper technical person before you use the product because may be caused damage.
- Keep away the product from heat sources.
- Save this document for future reference.
- Be careful when children are nearby and do not allow the children to play with the product.
- Do not exceed the maximum payload.
- Special care is always required where there are moving

parts that can cause limb entrapment and injury.

- 1 Do not attempt to lift the product by any removable parts.
- Do not use the product seat for a different purpose from the intended one.
- The lifting poles are not intended to carry the full weight of an individual.

DECLARATION OF CONFORMITY:

We are solely responsible for declaring that the Medical Devices mentioned in this statement are of Low-Risk Class (Class I) and comply with the requirements of the European Regulation 745/2017 and where appropriate, the standards and legislation referred to.

BEFORE USE:

 Check if the frame is damaged in order to guarantee a safe use of the product. (There are no cracks or fractures in the frame).

• In case of damage do not use the product and contact your dealer for further instructions.

 Check, if the product is properly assembled and all screws are secure and well screwed on.

 Always check the condition of wear for the mechanical parts to ensure the absolute safe use of the product for people and objects

ENVIRONMENTAL PROTECTION:

If one day you find that your product needs to be replaced or it is no longer working for you, consider protecting the environment: 1) Do not dispose your product along with the rest of the public waste (this is also the meaning of the shown recycling sign).

2) Contact your Public Authorities and they will instruct you of the Recycling centers to which your product must be disposed.

 Correct disposal of your product helps the protection of the environment as well as the recycling of the product's components.

MAINTENANCE, CLEANING & DISINFECTION INFORMATION:

To guarantee a safe use and adequate standard of hygiene, the user should perform these procedures before every use.

The user has to make certain of the structural integrity of the device and its components. For cleaning and sanitation procedures, follow the steps below:

1. Gloves should be worn.

Remove the evident dirt before to proceed with the most accurate disinfection.

- 3. Use water or mild detergent for the cleaning procedure.
- 4. Wipe with a dry and clean cloth.
- 5. DO NOT leave the product wet.

6. Do not use chemical cleaners to clean the frame. This could cause damage to the surface of the product

If you need to disinfect the product, use a common, mild disinfectant

8. Protect the item from scratches, cuts and punctures.

 Lubrication: the product has designed for a minimal maintenance; however, check every six months the lubrication on the moving & mechanical parts, this would ensure an optimal duration.

ASSEMBLING:

NOTE: The illustrations for the assembly are indicative to make the assembly easier. May will be differences from reality.


The support with LW10207 base is delivered disassembled and requires the following assembly operations:

1. Use 2*M10*115mm screws to fix the straight tube between the left and right leg tubes?



nsert the lifting pole in the space provided, and use plastic screw to fixed;

3. Insert the triangle with adjustable strap into the space provided.

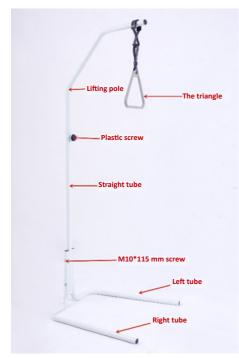

SYMBOL LEGEND

	Manufacturer
~	Date of manufacture
REF	Product code
LOT	Lot number
EC REP	Authorized representative in the European community
	Caution: read instructions (warnings) carefully
I	Consult instructions for use
CE	Medical Device compliant with Regulation (EU) 2017/745
MD	Medical Device
UDI	Unique device identifier
X.	WEEE disposal
	Imported by

WARRANTY:

The product is guaranteed for a period of one (1) year from the purchasing date.

The warranty apply on factory defects & DOES NOT apply on damages resulting from misuse, poor maintenance, modification, overuse, or non-compliance with the product's operating instructions.

Also DOES NOT apply on the parts, that can wear out during use or over time. Damages or defects caused by natural disasters, unauthorized maintenance or repair, power supply problems (where applicable) & carriers are not covered by the warranty.

No service or spare part is applied unless it has been inspected by an authorized service department or the manufacturer of the product. Shipping costs for goods of warranty are to be paid by the end user- customer or by dealer.

GIMA WARRANTY TERMS

The Gima 12-month standard B2B warranty applies.

Disposal: The product must not be disposed of along with other domestic waste. The users must dispose of this equipment by bringing it to a specific recycling point for electric and electronic equipment.