




# GIMA

PROFESSIONAL MEDICAL PRODUCTS

**ALZAWATER CON VITE DI BLOCCAGGIO FRONTALE**  
**RAISED TOILET SEAT WITH FRONTAL LOCKING SCREW**  
**REHAUSSEUR WC AVEC VIS DE BLOCAGE FRONTAL**  
**ALZAWATER CON TORNILLO DE BLOQUEO FRONTAL**  
**TOILETTENSITZERHÖHUNG MIT FRONTALER**  
**SICHERUNGSSCHRAUBE**  
**ΑΝΥΨΩΤΙΚΟ ΛΕΚΑΝΗΣ ΜΕ ΜΠΡΟΣΤΙΝΗ ΒΙΔΑ ΚΛΕΙΔΩΜΑΤΟΣ**

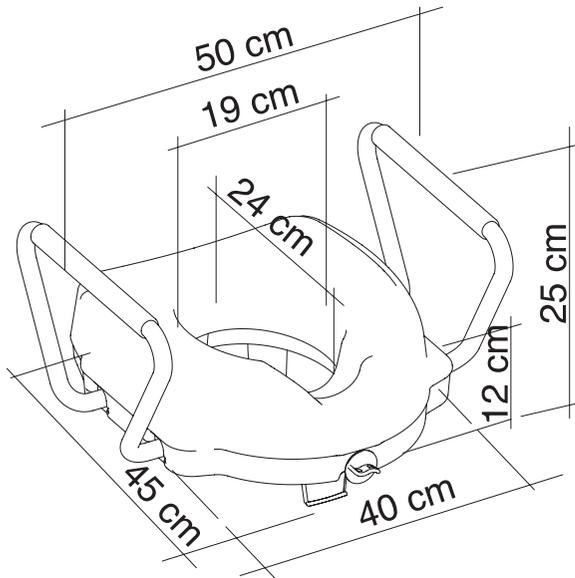

## ENGLISH

All serious accidents concerning the medical device supplied by us must be reported to the manufacturer and competent authority of the member state where your registered office is located.

### INTENDED USAGE

The products are designed to increase the height of the toilet bowl, in order to facilitate sitting down and getting up and to promote independence and comfort. The frontal locking system and the armrests make the use of the product safer.

### INDICATIONS AND CONTRAINDICATIONS

The Raised Toilet Seat is aimed to elderly people, wheelchair users, people with reduced mobility of lumbar, knee or hip and to all those who might have difficulty in sitting down and getting up from the toilet bowl. The version provided with folding armrests makes this Raised Toilet Seat particularly suitable for wheelchair users who resort to lateral transfer to the toilet seat. The ability to sit independently is required during the use. It is not recommended to use the Raised Toilet Seat in case of perception disorders or balance problems.

### SAFETY WARNINGS AND INDICATIONS

- The maximum user weight indicated in the fitting instructions must not be exceeded.
- Before every use, be sure the Raised Toilet Seat is in stable position on the WC and correctly fixed with the special fixing accessories supplied.
- The armrests must be properly assembled and, during use, the moving part must be correctly hooked as shown in the assembly pictures of the User Manual.
- During the assembly, strictly adhere to what is shown in the User Manual.
- Do not modify the Raised Toilet Seat and its components in any way.

- Do not use the Raised Toilet Seat if damaged or altered in any way. Cracks and deformations may strongly affect the performance and safety of the device.
- Be sure the height of the Raised Toilet Seat is such as to make the use of it easy and safe for the user.
- Do not lean on the Raised Toilet Seat while sitting or standing.
- During use, avoid positions that keep the body weight too much forward. Wrong positions may lead the user to slip and fall.
- The Raised Toilet Seat must not be stored outdoors.

### **MAINTENANCE INFO**

The products maintenance consists of the cleaning and sanitation procedures. In order to guarantee a safe use and adequate standard of hygiene, the user should perform these procedures before every use.

The user has to make certain of the structural integrity of the device and its components. For cleaning and sanitation procedures, follow the steps below:

1. Gloves should be worn.
2. Remove the evident dirt before to proceed with the most accurate disinfection.
3. Use water or non aggressive detergent for the cleaning procedure.
4. Wipe with a dry and clean cloth.

Alternatively, the Raised Toilet Seat can be cleaned in domestic dishwashers at the maximum temperature.

### **REUSE REQUIREMENTS**

The product is suitable for reuse by other users. Before reuse by others, the product must be correctly cleaned and sanitized. Before the transfer of the product to others, the product must be checked by qualified dealers.









### **CORRECT DISPOSAL PROCEDURE**

Do not dispose of the product in the normal household waste. Ask your local authority beforehand for the correct and environmentally friendly way to dispose it.

	Product code		Lot number
	Medical Device compliant with Regulation (EU) 2017/745		Manufacturer
	Serial number		Date of manufacture
	Medical Device		Consult instructions for use

### **GIMA WARRANTY TERMS**

The Gima 12-month standard B2B warranty applies.

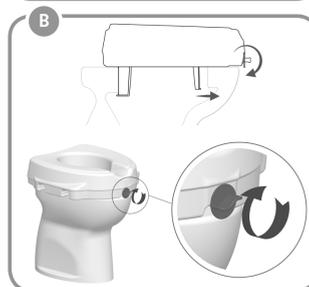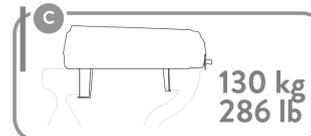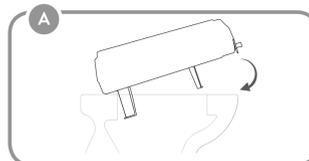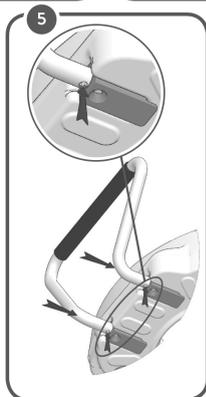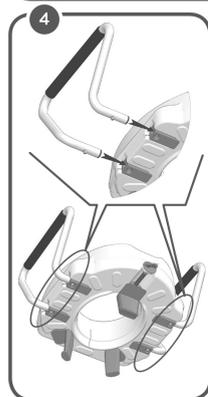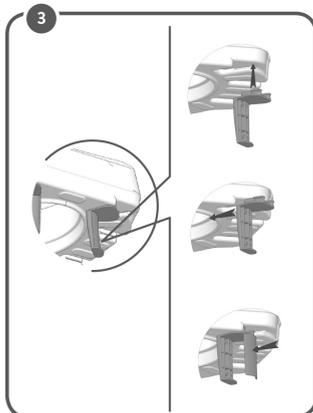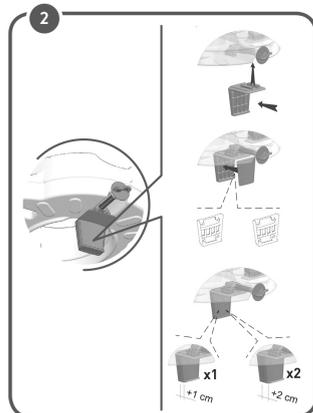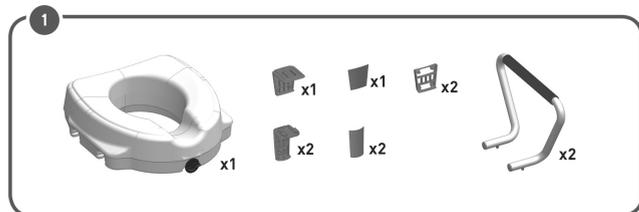

Carico massimo  
Max load  
Charge maximale  
Carga máxima



#### IT - LIMITE DI CARICO DEI BRACCIOLI:

**AVVERTENZA:** I braccioli servono ad aiutare l'utente a rimanere seduto in una posizione più riposante e fornire un ulteriore supporto sul quale è possibile scaricare parte del peso del corpo quando ci si siede o ci si alza. Tuttavia, non devono essere usati per appoggiarsi completamente a loro. Per un uso sicuro, non superare il carico massimo specifico raccomandato per i braccioli.

#### GB - ARMRESTS LOAD LIMIT:

**WARNING:** The armrests are meant to help the user to keep sitting in a more resting position and to provide a further support on which they can relieve part of the body weight when sitting down or standing up. However, they must not be used to completely lean on them. For a safe use, do not exceed the max load specifically recommended for the armrests.

#### FR - LIMITE DE CHARGE DES ACCOUDOIRS :

**MISE EN GARDE :** Les accoudoirs sont destinés à vous aider à rester assis dans une position plus reposante et à fournir un support supplémentaire sur lequel vous pouvez déléster une partie du poids du corps en vous asseyant ou en vous levant.

Cependant, veuillez ne pas les utiliser pour vous appuyer complètement dessus. Pour une utilisation en toute sécurité, ne dépassez pas la charge maximale spécifiquement recommandée pour les accoudoirs.

#### ES - LÍMITE DE CARGA DE LOS REPOSABRAZOS:

**ADVERTENCIA:** Los reposabrazos están destinados a ayudar al usuario a mantenerse sentado en una posición más en reposo y a proporcionar un soporte adicional en el que puedan aliviar parte del peso corporal al sentarse o ponerse de pie. Sin embargo, no deben utilizarse para apoyarse completamente en ellos. Para un uso seguro, no exceda la carga máxima recomendada específicamente para los reposabrazos.

#### DE - BELASTUNGSGRENZE DER ARMLEHNEN:

**WARNHINWEIS:** Die Armlehnen sollen dem Benutzer helfen, in einer bequemen Haltung zu sitzen und beim Hinsetzen oder Aufstehen einen Teil des Körpergewichts abstützen zu können. Trotzdem darf man sich nicht mit seinem ganzen Gewicht auf sie stützen. Für den sicheren Gebrauch dürfen Sie die speziell empfohlene maximale Last nicht überschreiten.

#### GR - ΟΡΙΟ ΒΑΡΟΥΣ ΣΤΗΡΙΓΜΑΤΩΝ ΒΡΑΧΙΟΝΑ:

**ΠΡΟΕΙΔΟΠΟΙΗΣΗ:** Σκοπός των στηριγμάτων βραχίονα είναι να διευκολύνουν τον χρήστη ώστε να κάθεται με πιο ξεκούραστο τρόπο καθώς και να παρέχουν περαιτέρω στήριξη επιτρέποντάς του να στηρίζει ένα μέρος του βάρους του όταν ετοιμάζεται να καθίσει ή να σηκωθεί. Ωστόσο, ο χρήστης δεν πρέπει να στηρίζεται εξ ολοκλήρου επάνω σε αυτά. Για ασφαλή χρήση, μην υπερβαίνετε το μέγιστο βάρος που αναφέρεται για τα στηρίγματα βραχίονα.

