



Disinfection process

1

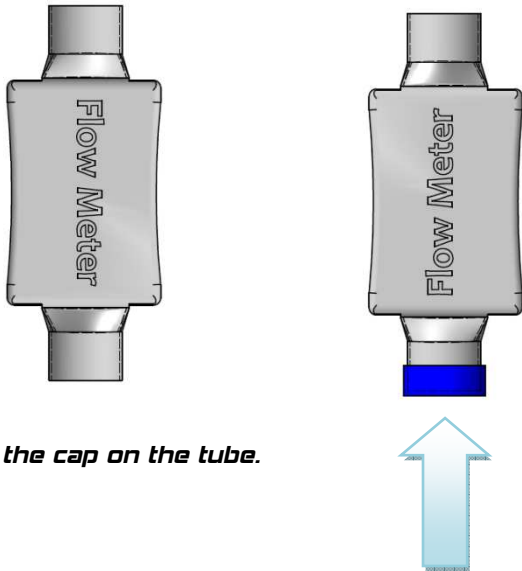

Put the cap on the tube.


2

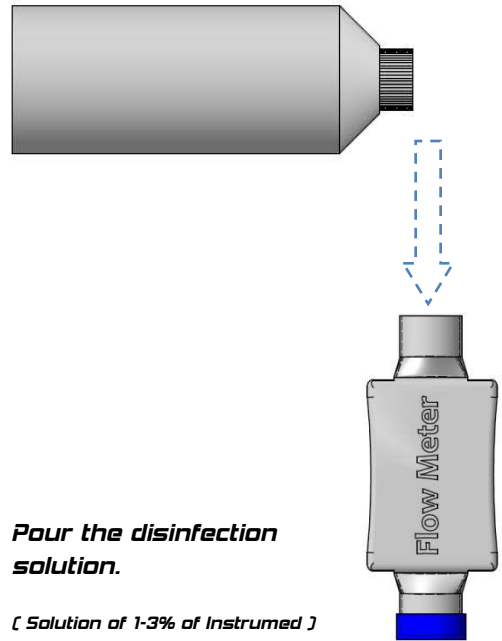

Pour the disinfection solution.

(Solution of 1-3% of Instrumed)

3

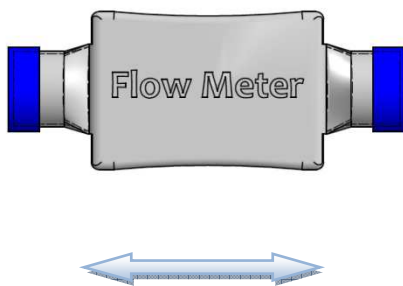

Put on the other cap and gently shake the flow meter.

4



Remove the caps.

Run water through the tube to clean it, and leave it to dry.