



GIMA

PROFESSIONAL MEDICAL PRODUCTS

TEST RAPIDO A CASSETTA PER LA MALARIA PLASMODIUM FALCIPARUM

MALARIA PLASMODIUM FALCIPARUM RAPID TEST CASSETTE

CASSETTE TEST RAPIDE POUR LE PALUDISME PLASMODIUM FALCIPARUM

CARTUCHO DE TEST RÁPIDO DE MALARIA PLASMODIUM FALCIPARUM

Manuale d'uso - User manual
Manuel de l'utilisateur - Guía de uso

PER USO PROFESSIONALE
FOR PROFESSIONAL USE
POUR USAGE PROFESSIONNEL
PARA USO PROFESIONAL

ATTENZIONE: Gli operatori devono leggere e capire completamente questo manuale prima di utilizzare il prodotto.

ATTENTION: The operators must carefully read and completely understand the present manual before using the product.

AVIS: Les opérateurs doivent lire et bien comprendre ce manuel avant d'utiliser le produit.

ATENCIÓN: Los operadores tienen que leer y entender completamente este manual antes de utilizar el producto.

GIMA 24547



Hangzhou AllTest Biotech Co., Ltd.
#550, Yinhai Street
Hangzhou Economic & Technological Development Area
Hangzhou - 310018, P.R. China
Made in China



IMA-402



MedNet GmbH
Borkstrasse 10 - 48163 Muenster, Germany

Importato da, imported by, importé par, importado por
Gima S.p.A.

Via Marconi, 1 - 20060 Gessate (MI) Italy
gima@gimaitaly.com - export@gimaitaly.com

www.gimaitaly.com



ENGLISH**Malaria P.f. Rapid Test Cassette**

(Whole Blood)

A rapid test for the qualitative detection of circulating plasmodium falciparum (P.f.) in human whole blood.
For professional in vitro diagnostic use only.

INTENDED USE

The Malaria P.f. Rapid Test Cassette (Whole Blood) is a rapid chromatographic immunoassay for the qualitative detection of circulating plasmodium falciparum in human whole blood.

SUMMARY

Malaria is caused by a protozoan which invades human red blood cells.¹ Malaria is one of the world's most prevalent diseases. According to the WHO, the worldwide prevalence of the disease is estimated to be 300-500 million cases and over 1 million deaths each year. Most of these victims are infants, young children. Over half of the world's population lives in malarious areas. Microscopic analysis of appropriately stained thick and thin blood smears has been the standard diagnostic technique for identifying malaria infections for more than a century.² The technique is capable of accurate and reliable diagnosis when performed by skilled microscopists using defined protocols. The skill of the microscopist and use of proven and defined procedures, frequently present the greatest obstacles to fully achieving the potential accuracy of microscopic diagnosis. Although there is a logistical burden associated with performing a time-intensive, labor-intensive, and equipment-intensive procedure such as diagnostic microscopy, it is the training required to establish and sustain competent performance of microscopy that poses the greatest difficulty in employing this diagnostic technology.
The Malaria P.f. Rapid Test Cassette (Whole Blood) is

a rapid test to qualitatively detect the presence of the P.f. antigen. The test utilizes colloid gold conjugate to selectively detect P.f. antigen in whole blood.

PRINCIPLE

The Malaria P.f. Rapid Test Cassette (Whole Blood) is a qualitative, membrane based immunoassay for the detection of P.f. antigen in whole blood. The membrane is pre-coated with P.f. antibody. During testing, the whole blood specimen reacts with the dye conjugate, which has been pre-coated in the test cassette. The mixture then migrates upward on the membrane chromatographically by capillary action and reacts with P.f. antibody on the membrane on the test line. If the specimen contains P.f. antigen, a colored line will appear in the test region. The absence of the colored line in test region indicates that the specimen does not contain P.f. antigen. To serve as a procedure control, a colored line will always appear in the control region indicating that proper volume of specimen has been added and membrane wicking has occurred.

REAGENTS

The test cassette contains anti-HRP-II of Plasmodium falciparum antibodies conjugated gold and anti-HRP-II antibodies coated on the membrane

PRECAUTIONS

- For professional in vitro diagnostic use only. Do not use after the expiration date.
- For whole blood specimen use only. Do not use other specimens.
- Do not eat, drink or smoke in the area where the specimens or kits are handled.
- Handle all specimens as if they contain infectious agents. Observe established precautions against microbiological hazards throughout all procedures and follow the standard procedures for proper disposal of specimens.
- Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are assayed.
- The used test should be discarded according to local regulations.
- Humidity and temperature can adversely affect results.

STORAGE AND STABILITY

The kit can be stored at room temperature or refrigerated (2-30°C). The test Cassette is stable through the expiration date printed on the sealed pouch. The test Cassette must remain in the sealed pouch until use. DO NOT FREEZE. Do not use beyond the expiration date.

SPECIMEN COLLECTION AND PREPARATION

- The Malaria P.f. Rapid Test Cassette (Whole Blood) can be performed using whole blood.
- Both Fingerstick Whole Blood and Venipuncture Whole Blood can be used.
- To collect Fingerstick Whole Blood specimens:
 1. Wash the patient's hand with soap and warm water or clean with an alcohol swab. Allow to dry.
 2. Massage the hand without touching the puncture site by rubbing down the hand towards the fingertip of the middle or ring finger
 3. Puncture the skin with a sterile lancet. Wipe away the first sign of blood.
 4. Gently rub the hand from wrist to palm to finger to form a rounded drop of blood over the puncture site.

- Testing should be performed immediately after specimen collection. Do not leave the specimens at room temperature for prolonged periods. Whole blood collected by venipuncture should be stored at 2-8°C if the test is to be run within 2 days of collection. For long term storage, specimens should be kept below -20°C. Whole blood collected by fingerstick should be tested immediately.
- Bring specimens to room temperature prior to testing. Frozen specimens must be completely thawed and mixed well prior to testing. Specimens should not be frozen and thawed repeatedly for more than three times.
- If specimens are to be shipped, they should be packed in compliance with federal regulations covering the transportation of etiologic agents.

MATERIALS

Materials Provided

- Test cassettes
- Disposable specimen droppers
- Buffer
- Package insert


Materials Required But Not Provided

- Pipette and disposable tips (optional)
- Specimen collection containers
- Lancets (for fingerstick whole blood only)
- Timer

DIRECTIONS FOR USE

Allow the test, specimen, buffer and/or controls to reach room temperature (15-30°C) prior to testing.

1. Bring the pouch to room temperature before opening it. Remove the test Cassette from the sealed pouch and use it as soon as possible.
2. Place the Cassette on a clean and level surface.
For Whole Blood specimen:
 - Use a pipette: To transfer 10µL of whole blood to the specimen well, then add 3 drops of buffer (approximately 180µL), and start the timer.
 - Use a disposal specimen dropper: Hold the dropper vertically; draw the specimen up to the Fill Line as shown in illustration below (approximately 10 µL). Transfer the specimen to the specimen well, then add 3 drops of buffer (approximately 180µL), and start the timer.
3. Wait for the colored line(s) to appear. Read results at 10 minutes. Do not interpret the result after 20 minutes.

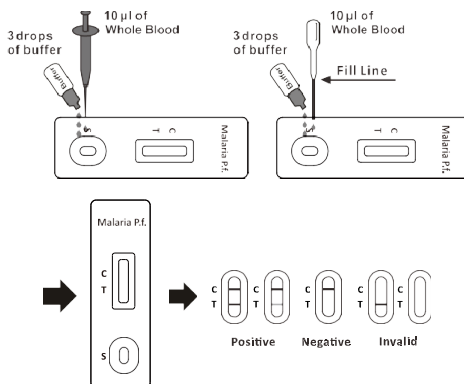

INTERPRETATION OF RESULTS

(Please refer to the illustration above)

POSITIVE: Two colored lines appear. One colored line should be in the control line region (C) and another colored line should be in the test line region (T).

***NOTE:** The intensity of the color in the test line region (T) will vary depending on the concentration of antigen, vis., HRP-II present in the specimen. Therefore, any shade of color in the test line region (T) should be considered positive.

NEGATIVE: One colored line appears in the control line region (C). No line appears in the test line region (T).

INVALID: Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

QUALITY CONTROL

Internal procedural controls are included in the test. A colored line appearing in the control region (C) is an internal valid procedural control. It confirms sufficient specimen volume and correct procedural technique.

Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

LIMITATIONS

1. The Malaria P.f. Rapid Test Cassette (Whole Blood) is for in vitro diagnostic use only. This test should be used for the detection of P.f. antigen in whole blood specimens only. Neither the quantitative value nor the rate of increase in P.f. antigen concentration can be determined by this qualitative test.
2. The Malaria P.f. Rapid Test Cassette (Whole Blood) will only indicate the presence of P.f. antigen the specimen and should not be used as the sole criteria for the diagnosis of malaria infection.
3. As with all diagnostic tests, all results must be interpreted together with other clinical information available to the physician.
4. If the test result is negative and clinical symptoms persist, additional testing using other

PERFORMANCE CHARACTERISTICS

Sensitivity and Specificity

The Malaria P.f. Rapid Test Cassette (Whole Blood) uses an antibody that is highly specific for Malaria P.f. antigen in whole blood. The Malaria P.f. Rapid Test Cassette (Whole Blood) has been tested with thin or thick blood smears on clinical samples. The results show that the sensitivity of the Malaria P.f. Rapid Test Cassette (Whole Blood) is over 99.0% relative to blood smears. And the results show that the specificity of the Malaria P.f. Rapid Test Cassette (Whole Blood) is >99% relative to blood smears.

Method		Blood Smears Microscopy		Total Results
Malaria P.f. Rapid Test Cassette (Whole Blood)	Results	Positive	Negative	
	Positive	90	0	90
	Negative	0	467	467
Total Results		90	467	557

Relative sensitivity: >99.9% (95%CI*: 96.7%~100.0%);
Relative specificity: >99.9% (95%CI*: 99.4%~100.0%);
Accuracy: >99.9% (95%CI*: 99.5%~100.0%).

*Confidence Intervals

Precision Intra-Assay

Within-run precision has been determined by using 15 replicates of three specimens: negative, low titer positive and high titer positive specimens. The specimens were correctly identified >99% of the time.

Inter-Assay

Between-run precision has been determined by 15 independent assays on the same three specimens: negative, low titer positive and high titer positive specimens. Three different lots of the Malaria P.f. Rapid Test Cassette (Whole Blood) have been tested using these specimens. The specimens were correctly identified >99% of the time.

Cross-reactivity

The Malaria P.f. Rapid Test Cassette (Whole Blood) has been tested by HAMA, RF, HBsAg, HBsAb, HBeAg, HBeAb, HBcAb, Syphilis, HIV, HCV, H.Pylori, MONO, CMV, Rubella and TOXO positive specimens. The results showed no cross-reactivity.

Interfering Substances

The following potentially interfering substances were added to Malaria negative and positive specimens.

- Acetaminophen: 20 mg/dL
- Caffeine: 20 mg/dL
- Acetylsalicylic Acid: 20 mg/dL
- Gentisic Acid: 20 mg/dL
- Ascorbic Acid: 2g/dL
- Albumin: 2 g/dL
- Creatin: 200 mg/dL
- Bilirubin: 1 g/dL
- Oxalic Acid: 60 mg/dL

None of the substances at the concentration tested interfered in the assay.

BIBLIOGRAPHY

1. Bill MacConell, Malaria Laboratory Diagnosis. January 2001
2. Cooke AH, Chiodini PL, Doherty T, et al, Comparison of a parasite lactate dehydrogenase-base immunochromatographic antigen detection assay with microscopy for the detection of malaria parasite in human blood samples. Am J Trop Med Hyp.1999, Feb: 60(2):173-2

Index of Symbols

	Keep away from sunlight
	Keep in a cool, dry place
	Please read instructions carefully
	Contains sufficient for "n" tests
	Disposable device, do not re-use
	In vitro diagnostic medical device compliant with Directive 98/79 / EC

	For in Vitro diagnostic use only
	Read instructions carefully
	Store between 2 and 30°C
	Authorized representative in the European community
	Expiration date (see box / package)
	Product code
	Lot number (see box / package)
	Manufacturer
	Do not use if package is damaged

GIMA WARRANTY TERMS

The Gima 12-month standard B2B warranty applies

Number: 145019602 Revision date: 2023-07-05