



GIMA

PROFESSIONAL MEDICAL PRODUCTS

PULSOXIMETRO OXY 9 - wireless
OXY 9 OXIMETER - wireless
OXYMÈTRE OXY 9 - sans fil
OXY 9 OXÍMETRO - inalámbrico
OXY 9 OXYMETER - kabellos
OXY 9 OXÍMETRO - sem fio

Gima 35078



CONTEC MEDICAL SYSTEMS CO., LTD
No.112 Qinhuang West Street,
Economic & Technical Development Zone,
Qinhuangdao, Hebei Province,
PEOPLE'S REPUBLIC OF CHINA
E-mail: med@eulinx.eu
Made in China



REF CMS50D-BT



Prolinx GmbH Brehmstr. 56,40239,
Duesseldorf, Germany

IP22



Importato da / Imported by / Importé par /
Importado por / Importado por / Eingeführt von:
Gima S.p.A.

Via Marconi, 1 - 20060 Gessate (MI) Italy
gima@gimaitaly.com - export@gimaitaly.com

www.gimaitaly.com



USER NOTICE

Dear users, thank you very much for purchasing the Pulse Oximeter(hereinafter referred to as device).

This Manual is written and compiled in accordance with the council directive MDD93/42/EEC for medical devices and harmonized standards. In case of modifications and software upgrades, the information contained in this document is subject to change without notice.

It is a medical device, which can be used repeatedly.

The Manual describes, in accordance with the device's features and requirements, main structure, functions, specifications, correct methods for transportation, assembly, usage, operation, repair, maintenance and storage, etc. as well as the safety procedures to protect both the user and device. Refer to the respective chapters for details.

Please read the User Manual carefully before using this device. The User Manual which describes the operating procedures should be followed strictly. Failure to follow the User Manual may cause measuring abnormality, device damage and human injury. The manufacturer is NOT responsible for the safety, reliability and performance issues and any monitoring abnormality, human injury and device damage due to users' negligence of the operation instructions. The manufacturer's warranty service does not cover such faults.

Owing to the forthcoming renovation, the specific products you received may not be totally in accordance with the description of this User Manual. We would sincerely regret for that.

Our company has the final interpretation to this manual. The content of this manual is subject to change without prior notice.

Warnings

Remind that it may cause serious consequences to tester, user or environment.

- ⚠ Explosive hazard—DO NOT use the device in environment with inflammable gas such as anesthetic.
- ⚠ DO NOT use the device while examining by MRI or CT, as the induced current may cause burn.
- ⚠ Do not take the information displayed on the device as the sole basis for clinical diagnosis. The device is only used as an auxi-



liary means in diagnosis. And it must be used in conjunction with doctor's advice, clinical manifestations and symptoms.

- The maintenance to the device can only be performed by qualified service personnel specified by manufacturer, Users are not permitted to maintain or refit the device by themselves. Unauthorized modification of the device would result unacceptable risk.
- Uncomfortable or painful feeling may appear if using the device ceaselessly, especially for the microcirculation disturbance users. It is not recommended that the sensor is used on the same finger for more than 2 hours.
- For some special users who need a more careful inspection on the test site, please don't place the device on the edema or tender tissue.
- Please do not stare at the red and infrared light emitter (the infrared light is invisible) after turning on the device, including the maintenance staff, as it may be harmful to the eyes.
- Each part of the device is firmly fixed,if accidental falling leads to the small parts such as a button to fall off,avoid swallowing of these parts,it may cause suffocation.
- The device contains silicone, PVC, TPU, TPE and ABS materials, whose biocompatibility has been tested in accordance with the requirements in ISO 10993-1, and it has passed the recommended biocompatibility test. The person who is allergic to silicone, PVC, TPU, TPE or ABS can not use this device.
- Do NOT strand the lanyard to avoid device drop and damage. The lanyard is made of insensitive material. Please do not use it if any person is allergic to lanyard. Do not wrap the lanyard around neck to avoid an accident.
- The disposal of scrap device, its accessories and packaging should follow the local laws and regulations, to avoid polluting to the local environment. And the packaging materials must be placed in the region where the children are out of reaching.
- The device can not be used with the equipment not specified in the Manual. Only the accessories appointed or recommended by the manufacturer can be used, otherwise it may cause injury to the tester and operator or damage to the device.
- Check the device before use to make sure that there is no



visible damage that may affect user's safety and device performance. When there is obvious damage, please replace the damaged parts before use.

- Functional testers can not be used to assess the accuracy of the Pulse Oximeter.
- Some functional testers or patient simulators can be used to verify whether the device works normally, for example, INDEX-2LFE Simulator (software version: 3.00), please refer to the Manual for the detailed operation steps.
- Some functional testers or patient simulators can measure the accuracy of the device copied calibration curve, but they can not be used to evaluate the device accuracy.
- When using the device, please keep it away from the equipment which can generate strong electric field or strong magnetic field. Using the device in an inappropriate environment may cause interference to the surrounding radio equipment or affect its working.
- When storing the device, keep it away from children, pets and insects to avoid affecting its performance.
- Do not place the device in places exposed to direct sunlight, high temperature, humidity, dust, cotton wool or easy to splash water, to avoid affecting its performance.
- The measured accuracy will be affected by the interference of electrosurgical equipment.
- When several products are used on the same patient simultaneously, danger may occur which is arisen from the overlap of leakage current.
- CO poisoning will appear excessive estimation, so it is not recommended to use the device.
- This device is not intended for treatment.
- The intended operator of the device may be a patient.
- Avoid maintaining the device during using.
- Users should read the product manual carefully before use and operate according to the requirements.

1 OVERVIEW

The oxygen saturation is the percentage of HbO₂ in the total Hb in the blood, so-called the O₂ concentration in the blood, it is an important physiological parameter for the respiratory and circulatory system. A number of diseases related to respiratory



system may cause the decrease of SpO₂ in the blood, furthermore, some other causes such as the malfunction of human body's self-adjustment, damages during surgery, and the injuries caused by some medical checkup would also lead to the difficulty of oxygen supply in human body, and the corresponding symptoms would appear as a consequence, such as vertigo, impotence, vomit etc. Serious symptoms might bring danger to human's life. Therefore, prompt information of patients' SpO₂ is of great help for the doctor to discover the potential danger, and is of great importance in the clinical medical field.

Insert the finger when measuring, the device will directly display the SpO₂ value measured, it has a higher accuracy and repeatability.

1.1 FEATURES

A. Easy to use.

B. Small in volume, light in weight, convenient to carry.

C. Low power consumption.

1.2 INTENDED PURPOSE

The Fingertip Pulse Oximeter is a non-invasive device intended for the spot-check of oxygen saturation of arterial hemoglobin (SpO₂) and the pulse rate of adult and pediatric patients in home and hospital environments (including clinical use in internist/surgery, anesthesia, intensive care ect.). This device is not intended for continuous monitoring.

1.3 ENVIRONMENT REQUIREMENTS

Storage Environment

a) Temperature: -40°C ~ + 60°C

b) Relative humidity: ≤ 95%

c) Atmospheric pressure: 500 hPa ~ 1060 hPa

Operating

a) Temperature: +10°C ~ + 40°C

b) Relative Humidity: ≤ 75%

c) Atmospheric pressure: 700 hPa ~ 1060 hPa

1.4 PRECAUTIONS

1.4.1 Attention

Point out conditions or practices that may cause damage to the device or other properties.

 Before using the device, make sure that it locates in normal



working state and operating environment.

-  In order to get a more accurate measurement, it should be used in a quiet and comfortable environment.
-  When the device is carried from cold or hot environment to warm or humid environment, please do not use it immediately, wait four hours at least is recommended.
-  If the device is splashed or coagulated by water, please stop operating.
-  DO NOT operate the device with sharp things.
-  High temperature, high pressure, gas sterilizing or immersion disinfection for the device is not permitted. Refer to User Manual in the relative chapter (6.1) for cleaning and disinfection. Please take out the internal battery before cleaning and disinfection
-  The device is suitable for adult.
-  The device may not be suitable for all users, if you can't get a satisfactory result, please stop using it.
-  Data averaging and signal processing have a delay in the upgrade of SpO2 data values. When the data update period is less than 30 seconds, the time for obtaining dynamic average values will increase, which is arisen from signal degradation, low perfusion or other interference, it depends on the PR value.
-  The device has 3-year service life, date of manufacture sees the label.
-  The device does not provide over-limit alarm function for SpO2 and PR, so it is inapplicable for using in the place where need such function.
-  The device hasn't low-voltage alarm function, it only shows the low-voltage, please change the battery when the battery voltage is used up.
-  The maximum temperature at the SpO2 probe -tissue interface should be less than 41°C which is measured by the temperature tester.
-  During measuring, when abnormal conditions appear on the screen, please pull out your finger and reinsert it to measure again.
-  If some unknown error appears during measuring, remove the battery to terminate operating.



-  Do not contort or drag the wire of the device.
-  The plethysmographic waveform is not normalized, as a signal inadequacy indicator, when it is not smooth and stable, the accuracy of the measured value may degrade. When it tends to be smooth and stable, the measured value read is the optimal and the waveform at this time is also the most standard.
-  If the device or component is intended for single-use, then the repeated use of these parts will pose risks on the parameters and technical parameters of the equipment known to the manufacturer.
-  If necessary, our company can provide some information (such as circuit diagrams, component lists, illustrations, etc.), so that the qualified technical personnel of the user can repair the device components designated by our company.
-  Operators can contact our company to obtain the modified Bland and Altman plot.
-  The measured results will be influenced by the external colouring agent (such as nail polish, colouring agent or color skin care products, etc.), so don't use them on the test site.
-  Do not fix the SpO2 sensor with adhesive or else it may result in venous pulsation and inaccurate measure of SpO2 and pulse rate.
-  As to the fingers which are too cold or too thin or whose fingernail is too long, it may affect the measured results, so please insert the thicker finger such as thumb or middle finger deeply enough into the probe when measuring.
-  The finger should be placed correctly (see Attached figure 5), as improper assembly or improper contact position for sensor will influence the measurement.
-  The light between the photoelectric receiving tube and the light-emitting tube of the device must pass through the subject's arteriole. Make sure the optical path is free from any optical obstacles like rubberized fabric, to avoid inaccurate results.
-  Excessive ambient light may affect the measured results, such as surgical light (especially xenon light sources), bilirubin lamp, fluorescent lamp, infrared heater and direct sunlight, etc. In order to prevent interference from ambient



light, make sure to place the sensor properly and cover the sensor with opaque material.

-  Frequent movement (active or passive) of the subject or severe activity can affect the measured accuracy.
-  The Pulse Oximeter should not be placed on a limb with the blood pressure cuff, arterial ductus or intraluminal tube.
-  The measured value may be inaccurate during defibrillation and in a short period after defibrillation, as it has not defibrillation function.
-  The device has been calibrated before leaving factory.
-  The device is calibrated to display functional oxygen saturation.
-  The equipment connected with the Oximeter interface should comply with the requirements of IEC 60601-1.

1.4.2 Clinical restriction

- A. As the measure is taken on the basis of arteriole pulse, substantial pulsating blood flow of subject is required. For a subject with weak pulse due to shock, Raynaud's syndrome, low ambient/body temperature, major bleeding, or use of vascular contracting drug, the SpO₂ waveform (PLETH) will decrease. In this case, the measurement will be more sensitive to interference.
- B. The measurement will be influenced by intravascular staining agents (such as indocyanine green or methylene blue), skin pigmentation.
- C. The measured value may be normal seemingly for the tester who has anemia or dysfunctional hemoglobin (such as carboxyhaemoglobin (COHb), methaemoglobin (MetHb) and sulphaemoglobin (SuHb)), but the tester may appear hypoxia, it is recommended to perform further assessment according the clinical situations and symptoms.
- D. Pulse oxygen only has a reference meaning for anemia and toxic hypoxia, as some severe anemia patients still show better pulse oxygen measured valued.
- E. Contraindication:
 - a. The person who is allergic to silicone, PVC, TPU TPE or ABS.
 - b. The damaged skin tissue.
 - c. During cardiopulmonary resuscitation.
 - d. When the patient is hypovolemic.
 - e. For assessing the adequacy of ventilatory support.

- f. For detecting worsening lung function in patients on a high concentration of oxygen.

1.5 CLINICAL INDICATIONS

The Pulse Oximeter can be used in measuring the pulse oxygen saturation and pulse rate through finger.

2 PRINCIPLE

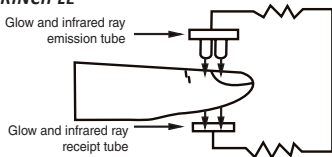


Figure 1. Operating principle

An experience formula of data processing is established taking use of Lambert Beer Law according to Spectrum Absorption Characteristics of Reductive Hemoglobin (Hb) and Oxyhemoglobin (HbO₂) in red light & near-infrared light zones. On the basis of the principle of Photoelectric Oxyhemoglobin Inspection Technology and Photoplethysmography technology, it uses two light beams of different wavelengths to irradiate the human fingertip to obtain the measurement information from the photosensitive element, after processed by the electronic circuits and micro-processor, displays the measured results on the screen.

3 FUNCTIONS

- A. SpO₂ value display
- B. PR value and bar graph display.
- C. Pulse waveform display
- D. Low-voltage indication: low-battery indication appears when the battery voltage is too low to work.
- E. Display direction can be changed automatically.
- F. Automatic standby function.
- G. Memory function.
- H. The data can be uploaded to the terminal equipment by wireless mode
- I. Display mode can be changed

4 PRODUCT INTRODUCTION

4.1 VIEW OF THE FRONT PANEL




Figure 2. Front view

Button: exit standby;

4.2 BATTERY ASSEMBLY

- Refer to Figure 3 open the battery compartment cover on the back of the device, and insert the two AAA size batteries properly in the right direction.
- Replace the cover.

Attention: Please take care when you insert the batteries for the improper insertion may damage the device.

Attention: Please replace two new batteries of the same kind at the same time.



Figure 3



Figure 4

4.3 ACCESSORIES

- Put the thinner side of the rope through the hole (see Figure 4).
- Put the wider side of the rope through the thinner side which has been put through the hole, then tighten it.

4.4 STRUCTURE, ACCESSORIES AND SOFTWARE DESCRIPTION

- Structure: main unit
- Accessories: one hanging, one CD disk (including PC software, optional).

Attention: Please check the device and accessories according to the list to avoid that the device can not work normally.



C. Software description

Release version:V2

5 OPERATING GUIDE

5.1 APPLICATION METHOD

A. Measurement and Data storage

- a) Insert the two batteries properly to the direction, and then replace the cover.
- b) Open the clip as shown in Figure 5.
- c) Let the user's finger put into the rubber cushions of the clip (make sure the finger is in the right position), and then clip the finger.
- d) Do not shake the finger and keep the user in a stable state during the process.
- e) Press "Button" to exit from the standby mode. The data can be read directly from the screen on the measuring interface.



Figure 5 Put finger in position



Figure 6 Synchronous time interface

- 1) Enter to "Synchronous Time..." interface (as Figure 6).
- 2) Three methods to exit from "Synchronous Time..." interface.

The first method:

Don't perform sync time, press the button, then the device will enter to measurement interface from "Synchronous Time..." interface.

The second method:

Don't perform sync time, wait for several minutes, then the device will enter to measurement interface from "Synchronous Time..." interface.

The third method:

Perform sync time, connect to power, then the device will turn on

automatically, when it enters to "Synchronous Time..." interface, connect it with App, then it will automatically adjust time.

Attention: Fingernails and the luminescent tube should be on the same side.

Attention: If the prompt function is on, the device will provide medium-priority prompt signal when finger is out. Intermittent prompt will occur and the user interface presents "FINGER OUT". Medium priority indicating that prompt operator response is required.

Attention: Please synchronize the time with the master device when using it for the first time or after replacing batteries, refer to chapter 5.1.A.e) for relative operations.

- B. The device could change display direction according to the handing direction.
- C. Start recording after stable data appear, pull out the finger to finish recording a group of data
- D. Under non-measurement state, it will enter standby mode automatically when there is no operation within 1 min.

5.2 DATA UPLOAD

Turn on the device Bluetooth and the PC software to upload data, refer to "Software operating instruction" for details.

6 MAINTAIN, TRANSPORTATION AND STORAGE

6.1 CLEANING AND DISINFECTING

The device must be turned off before cleaning, and it should not be immersed into liquid.

Please take out the internal battery before cleaning, do not immerse it into liquid.

Use 75% alcohol to wipe the device enclosure and the nail pad, nature dry or clean it with clean and soft cloth. Do not spray any liquid on the device directly, and avoid liquid penetrating into the device.

6.2 MAINTAIN

- A. Check the main unit and all accessories periodically to make sure that there is no visible damage that may affect patient's safety and monitoring performance. It is recommended that the device should be inspected weekly at least. When there is obvious damage, stop using it.
- B. Please clean and disinfect the device before/after using it according to the User Manual (6.1).



- C. Please replace the batteries in time when low-battery appears
- D. Please take out the batteries if the device is not used for a long time.
- E. The device need not to be calibrated during maintenance.

6.3 TRANSPORTATION AND STORAGE

- A. The packed device can be transported by ordinary conveyance or according to transport contract. During transportation, avoid strong shock, vibration and splashing with rain or snow, and it can not be transported mixed with toxic, harmful, corrosive material .
- B. The packed device should be stored in room with no corrosive gases and good ventilation. Temperature: $-40^{\circ}\text{C} \sim +60^{\circ}\text{C}$; Relative humidity: $\leq 95\%$

7 TROUBLESHOOTING

Trouble	Possible Reason	Solution
The values can not be displayed normally or stably	1) The finger is not properly inserted. 2) The finger is shaking or the patient is moving. 3) The device is not used in environment required by the manual. 4) The device works abnormally.	1) Please insert the finger properly and measure again. 2) Let the patient keep calm. 3 Please use the device in normal environment. 4 Please contact the after-sales.
The device can not be turned on	1) The battery is drained away or almost drained away. 2) The battery is assembled incorrectly. 3) The device's malfunction.	1) Please change batteries. 2) Please assemble the battery again. 3) Please contact the local service center.
The display disappears suddenly.	1) The device enters into the energy saving mode. 2) Low battery. 3) The device works abnormally.	1) Normal. 2) Please change batteries. 3) Please contact the after-sale
The data can not be stored.	1 The device is not operated according to the manual. 2 The device works abnormally.	1 Please operate the device according to the manual. 2 Please contact the after-sales.

8 SYMBOLS

Symbols	Meaning	Symbols	Meaning
	Follow instructions for use	PR bpm	Pulse rate (bpm)
	Type BF applied part	% SpO₂	Pulse oxygen saturation (%)
	Manufacturer		Fully charged
SN	Serial number		Low battery
	WEEE disposal		Battery cathode
+	Battery anode	Synchronous Time...	Synchronous time interface
	Manufacture Date		Humidity limitation
	Temperature limitation		This side up
	Atmospheric pressure limitation		Keep away from rain
	Fragile, handle with care		Bluetooth icon
	Power button	LOT	Lot number
	Recyclable	Finger Out	The finger is not inserted.
	Use-by date	EU REP	European Representative
	Alarm inhibit		Caution
P/N	Material code		Stacking limit by number
MD	Medical device	UDI	Unique device identification



REF	Product code	---	1. The finger clip falls off (no finger inserted) 2. Signal inadequacy indicator
CE	This item is compliant with Directive 93/42/EEC of 14 june 1993 concerning medical devices; Including, at 21 march 2010, the amendments by Council Directive 2007/47/EC.		
IP22	It means this pulse oximeter is protection against ingress of solid foreign objects of 12.5mm and greater, protection against ingress of water dripping when device tilted up to 15°.		

Note: Your device may not contain all the following symbols.

9 SPECIFICATION

SpO2 [see note 1]	
Display range	0% ~ 99%
Measured range	0% ~ 100%
Accuracy [see note 2]	70%~100%: $\pm 2\%$; 0%~69%: unspecified.
Resolution	1%
PR	
Display range	30 bpm ~ 250 bpm
Measured range	30 bpm ~ 250 bpm
Accuracy[see note 3]	± 2 bpm during the pulse rate range of 30 bpm ~ 99 bpm and $\pm 2\%$ during the pulse rate range of 100 bpm ~ 250 bpm.
Resolution	1 bpm
Accuracy under low perfusion [see note 4]	Low perfusion 0.4%: SpO2: $\pm 4\%$; PR: ± 2 bpm during the pulse rate range of 30 bpm ~ 99 bpm and $\pm 2\%$ during the pulse rate range of 100 bpm ~ 250 bpm.
Light interference	Under normal and ambient light conditions, the SpO2 deviation $\leq 1\%$
Pulse intensity	Continuous bar graph display, the higher display indicates the stronger pulse.
Optical sensor [see note 5]	
Red light	Wavelength: about 660 nm, optical output power: < 6.65 mW

Infrared light	Wavelength: about 905 nm, optical output power: < 6.75 mW
Memory	Store approximately 30 point of data
Safety class	Internally powered equipment, type BF applied part
International Protection	IP22
Working voltage	DC2.6V-3.6 V
Working current	≤ 100 mA
Power supply	1.5V (AAA size) alkaline batteries × 2
Operation time	The device can continuously work for 20 hours when it was powered by two new batteries within the warranty period.
Dimension and Weight	
Dimension	58(L) × 32(W) × 34 (H) mm
Weight	About 52g (with the batteries)

Note 1: the claims of SpO₂ accuracy shall be supported by clinical study measurements taken over the full range. By artificial inducing, get the stable oxygen level to the range of 70 % to 100 % SaO₂, compare the SpO₂ values collected by the secondary standard pulse oximeter equipment and the tested equipment at the same time, to form paired data, which are used for the accuracy analysis.

There are 12 healthy volunteers (male: 6. female: 6; age: 18~50; skin color: dark black: 3, medium dark: 1, light: 7, white: 1) data in the clinical report.

Note 2: because pulse oximeter equipment measurements are statistically distributed, only about two-thirds of pulse oximeter equipment measurements can be expected to fall within ±Arms of the value measured by a CO-OXIMETER.

Note 3: Patient simulator has been used to verify the pulse rate accuracy, it is stated as the root-mean-square difference between the PR measurement value and the value set by simulator.

Note 4: percentage modulation of infrared signal as the indication of pulsating signal strength, patient simulator has been used to verify the accuracy under conditions of low perfusion. SpO₂ and PR values are different due to low signal conditions, compare them with the known SpO₂ and PR values of input signal.

Note 5: optical sensors as the light-emitting components, will



affect other medical devices applied the wavelength range. The information may be useful for the clinicians who carry out the optical treatment. For example, photodynamic therapy operated by clinician.

EMC

This equipment is suitable for professional healthcare facility environments and home healthcare environments

Warning:

- ⚠ Don't near active HF SURGICAL EQUIPMENT and the RF shielded room of an ME SYSTEM for magnetic resonance imaging, where the intensity of EM DISTURBANCES is high.
- ⚠ Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.
- ⚠ Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.
- ⚠ Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the this equipment, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

Note:

- ⚠ This equipment needs special precautions regarding EMC and needs to be assembled and put into service according to the EMC information provided below.
- ⚠ The basic performance: SpO2 measured range: 70% ~ 100%, absolute error: $\pm 2\%$; PR measured range: 30 bpm ~ 250 bpm, accuracy: ± 2 bpm during the pulse rate range of 30 bpm ~ 99 bpm and $\pm 2\%$ during the pulse rate range of 100 bpm ~ 250 bpm.
- ⚠ When the device is disturbed, the data measured may fluctuate, please measure repeatedly or in another environment to ensure its accuracy.

- ⚡ Other devices may affect this device even though they meet the requirements of CISPR.

Bluetooth Specification

Working frequency: 2402 MHz ~ 2480 MHz

Modulation mode: GFSK

Transmitting power: 0 dBm, +4 dBm

Receiving sensitivity: -93 dBm

TABLE 1:

Guidance and Declaration - Electromagnetic Emissions	
Emission test	Compliance
Radiated RF EMISSIONS	Group 1
Radiated RF EMISSIONS	Class B
Harmonic distortion IEC 61000-3-2	Not applicable
Voltage fluctuations and flicker IEC 61000-3-3	Not applicable

TABLE 2:

Guidance and Declaration - Electromagnetic Immunity		
Immunity test	IEC60601 test level	Compliance level
Electrostatic discharge (ESD) IEC 61000-4-2	±8kV contact ±15 kV air	±8kV contact ±15kV air
Electrical fast transient/ burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/ output lines	Not Applicable
Surge IEC 61000-4-5:	±1 kV line(s) to line(s) ±2 kV line(s) to earth	Not Applicable
Voltage dips and Voltage interruptions IEC 61000-4-11	0%UT; 0,5 .cycle .At0°,45°,90°,135°,180°,225°, 270° and 315°. 0 % UT; 1 cycle and 70 % UT ; 25/30 cycles ; Single phase:at 0°. 0 % UT ; 250/300 cycle	Not Applicable
Power frequency(50/60Hz) magnetic field IEC 61000-4-8	30 A/m 50Hz/60Hz	30 A/m 50Hz/60Hz
Conducted RF IEC61000-4-6	3 V 0,15MHz - 80 MHz 6 V in ISM and amateur radio bands between 0,15MHz to 80 MHz 80%AM at 1kHz	Not Applicable



Radiated RF IEC61000-4-3	10V/m 80 MHz-2,7GHz 80%AM at 1kHz	10V/m 80 MHz-2,7GHz 80%AM at 1kHz
NOTE UT is the a.c.mains voltage prior to application of the test level		

TABLE 3:

Guidance and manufacturer's declaration - electromagnetic Immunity						
Radiated RF IEC61000-4-3 (Test specifications for ENCLOSURE PORT IMMUNITY to RF wire-less communications equipment)	Test Frequency (MHz)	Band (MHz)	Service	Modulation	IEC60601-1-2 Test level (V/m)	Compliance level (V/m)
	385	380 –390	TETRA 400	Pulse modulation b) 18 Hz	27	27
	450	430 –470	GMRS 460, FRS 460	FM c) ± 5 kHz deviation 1 kHz sine	28	28
	710	704 –787	LTE Band 13,17	Pulse modulation b) 217 Hz	9	9
	745					
	780					
	810	800 –960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation b) 18 Hz	28	28
	870					
	930					
	1720	1700 –1990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3,4,25; UMTS	Pulse modulation b) 217 Hz	28	28
	1845					
	1970					
	2450	2400 –2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation b) 217 Hz	28	28
	5240	5100 –5800	WLAN 802.11 a/n	Pulse modulation b) 217 Hz	9	9
	5500					
	5785					



Disposal: The product must not be disposed of along with other domestic waste. The users must dispose of this equipment by bringing it to a specific recycling point for electric and electronic equipment.

GIMA WARRANTY TERMS

The Gima 12-month standard B2B warranty applies.